Virto M – Order Form

Custom Hearing Instruments

PHONAK
life is on

Step 1 – General Information

Order No:_____

Date of Order:_____

Dispenser Name (BLOCK CAPITALS):

_____

Address:_____

_____

Patient Name (BLOCK CAPITALS):

_____

(AC & BC thresholds required for AOV)

		250	500	1000	2000	3000	4000	8000	
Left:	AC								dB
	BC								dB
Right:	AC								dB
	BC								dB
		Hz	Hz	Hz	Hz	Hz	Hz	Hz	

AC = Air Conduction Thresholds BC= Bone Conduction Thresholds

If there is a query with your order please list the most appropriate way(s) to contact you.

Tel:_____ Mobile:_____

Email:_____

Other:_____

Step 2 – Performance Level

Virto M-Titanium

☐ M90 ☐ M70

Virto M-10 NW 0 / M-312 NW 0 / M-312

☐ M90 ☐ M70 ☐ M50 ☐ M30

Step 3 – Product

For selection options and codes see combination matrix on the reverse.

Virto M-Titanium

☐ L ☐ R

Virto M-10 NW 0

☐ L ☐ R

Virto M-312 NW 0

☐ L ☐ R

Virto M-312

☐ L ☐ R

FitGuide values

L_____ R_____

Step 4 – Power Level

Left: ☐ M ☐ P ☐ SP ☐ UP*

Right: ☐ M ☐ P ☐ SP ☐ UP*

Step 5 – Colours

Shell

- ☐ 06 Black*
- ☐ 19 White
- ☐ 21 Transparent
- ☐ 22 Cocoa
- ☐ 26 Pink
- ☐ 28 Brown
- ☐ R/B Red/Blue
- ☐ U0 Titanium grey**

Faceplate

- ☐ 06 Black***
- ☐ 22 Cocoa
- ☐ 26 Pink
- ☐ 28 Brown

*Only for Virto M-312 directional **Only for Virto M-Titanium
***Not for Virto M-312 NW 0

Step 6 – Options

Fast Order ▶▶ Build product as standard version ☐

Legend ☐ / (S) = standard ▭ = optional

Shell size	Smallest possible	(S)
	Manually selected	Style:
Vent size	AOV (enter audiogram)	(S)
	Manually selected	Left: _____ mm
		Right: _____ mm
Wax system	Cerustop (CS)	(S)
	Manually selected	Type:
User controls	Standard controls	(S)
	EasyPhone & push button	☐
	EasyPhone without push button	☐
	MiniControl without push button	☐
	Volume control (VC)	☐
	T-coil	☐
Removal line (RF)	Transparent (21)*	☐
	Line extension +5 mm (RFE)	☐
Titanium surface	Extra retention (ERS)	☐
Accessories (Virto M-312)	TV Connector	☐
	Phonak Partner Mic™	☐
	Phonak RemoteControl	☐

*Standard for IIC & CIC

Special Instructions:_____

_____

_____

Virto M - Order Form

Custom Hearing Instruments

PHONAK
life is on

Combination Matrix

		Virto M-Titanium	Virto M-10 NW O	Virto M-312 NW O	Virto M-312
Shell style		IIC, CIC	IIC, CIC, M, C, HS, FS	M, C, HS, FS	HS, FS
Push button	Standard	No push button (PX)	Push button (PM1)	No push button (PX)	Push button (PM1)
	Optional	Push button (PM1)	No push button (PX)	Push button (PM1)	-
Volume Control	Standard	-	No VC (VCX)	No VC (VCX)	No VC (VCX)
	Optional	-	Digital VC (VC3)	Digital VC (VC3)	Digital VC (VC3)
T-Coil	Standard	No T-coil (TX)	No T-coil (TX)	No T-coil (TX)	-
	Optional	T-coil passive (TP)	T-coil passive (TP) (not available in combination with VC)	T-coil passive (TP) (not available in combination with VC)	-
Magnetic switch function	Standard	MiniControl (DT5)	EasyPhone (DT4)	EasyPhone (DT4)	-
	Optional	EasyPhone (DT6)	MiniControl (DT3) No magnetic switch (RX)	No magnetic switch (RX)	-
Wax system	Standard	Cerustop (CS)	Cerustop (CS)	Cerustop (CS)	Cerustop (CS)
	Optional	-	HF3 (H3) Extended rec. tube (ER) Wax Spring (WS) Ext. Tube + Spring (WE) Wax guard not required (X)	HF3 (H3) Extended rec. tube (ER) Wax Spring (WS) Ext. Tube + Spring (WE) Wax guard not required (X)	HF3 (H3) Extended rec. tube (ER) Wax Spring (WS) Ext. Tube + Spring (WE) Wax guard not required (X)
Removal line	Standard	Removal line transparent (RF)*	Removal line transparent (RF)*	-	-
	Optional	-	Removal line transparent (RF)	Removal line transparent (RF)	Removal line transparent (RF)

*IIC & CIC will be standardly equipt with removal line

Titanium Information

Vent Options

AOV = Acoustically Optimized Vent. Phonak will set the correct vent diameter and style in relation to Audiogram/shell geometry/ feedback canceler and required low frequency gain. This is the recommended vent type.

AOV-O = Acoustically Optimized Vent-Open. This specific vent is more open and recommended for first time users and clients who are sensitive to occlusion.
N.B. This option will increase the device size

Titanium FitGuide

Measure the possible insertion depth. The device will be built in accordance with the indicated FitGuide value. If the measurement falls between two numbers, please use the smaller number.

- Side M - For devices with M-receiver
- Side P - For devices with P-receiver
- Models with SP receiver will be built without FitGuide information

Impression Taking

Recommendation for taking deep impressions:
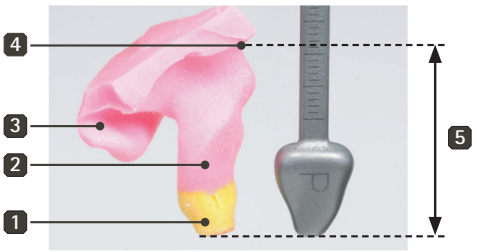
- Use EasyView Otoblock 1
- Use Dreve Otoform A softX 25 shore A (#2956) 2
- Always fill the complete concha with impression material 3
- Intertragal notch must be visible 4
- Impression length must cover the evaluated FitGuide value 5